


Monoflex™

INSTALLATION AND USER'S INSTRUCTIONS

ART NOS. SH120 & SH122

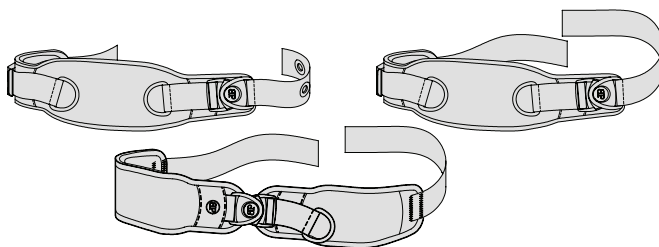

These instructions provide important information for the safe use and maintenance of all Bodypoint Monoflex™ Chest Belts. Give these instructions to the user or their caregiver and review them to ensure that they are understood.

⚠ WARNING! Product should be installed and fitted by a qualified rehab technician.

For installation, this product should be mounted with:

Flat-mount end-fittings

Cinch-mount end-fittings

Cam buckle (1" suitable for users up to 75kg, 1-1/2" and 2" suitable for all users)

Optional Bodypoint belt mounting hardware may be used for mounting to wheelchairs and seating systems.

⚠ WARNING! Because of the risk of choking, it is dangerous to use this product without stabilizing the pelvis – always use with a properly fitted pelvic support belt.

INTENDED USE:

⚠ WARNING! This product should only be used for positioning a person in a wheelchair or work chair. It is NOT intended for use as a transportation safety device, as a personal restraint device, or in any other application where its failure could result in injury. Misuse of this product is unauthorized and unsafe.

⚠ WARNING! This anterior trunk support must be properly fitted to support the user's trunk and shoulders without causing injury. Have your seating specialist demonstrate its proper adjustment and use.

- If it is too tight, it can restrict respiration and increase pressure across the shoulders and chest.
- If it is too loose, it can allow the user to slip down and may create a risk of strangulation.
- Accidental release of this product can allow the user to fall forward.
- A user's inability to self-release can be hazardous if the user slips down or is trapped in the wheelchair in an emergency.

If the user's physical or cognitive abilities could prevent them from safely operating this product, a caregiver must be present at all times during its use. Ensure that all caregivers know how to correctly adjust and unfasten the product.

⚠ WARNING! As with any new seating support, this product may change the way a person sits. Users must continue to practice regular pressure relief activities and skin integrity checks, not only where this product contacts the user, but also in primary pressure-bearing areas such as the sacrum, legs, and buttocks. If increased skin redness or irritation occurs, discontinue use and consult your physician or seating specialist. Failure to do so may result in serious injury, such as pressure ulcers.

⚠ WARNING! If a serious incident occurs related to the use of this product, it should be reported to the manufacturer (Bodypoint, Inc.) and the local Competent Authority.

PERIODIC SAFETY AND PERFORMANCE CHECKS:

To ensure user safety, this product must be checked periodically for function and signs of wear. If the product does not function correctly or if significant wear is found in the buckles, mounting points, webbing, padding, or stitches, stop using it and contact your supplier for qualified repair or replacement by Bodypoint. Under no circumstance should this product be altered or repaired by unqualified persons — health and safety depend on it!



CLEANING: Machine wash, hot, 60°C (140°F). Do not bleach. Tumble dry, low temperature, or drip dry. Do not iron. (Placing the product inside a cloth bag during washing helps prevent scratches to the product and the machine.)

SCRAP/DISPOSAL: Product is made of materials which can be disposed of safely without special precautions at the end of its useful life.

WARRANTY: This product carries a limited-life-time warranty against defects in workmanship and materials arising under normal use by the original consumer. Contact your supplier or Bodypoint for warranty claims.


For more information on Bodypoint products, and a list of distributors outside the USA, go to www.bodypoint.com



Bodypoint Europe BV
Kerkstraat 29
7396 PD Tenwolde
The Netherlands




558 First Ave. S., Suite 300 | Seattle, WA 98104 | 206.405.4555 | 800.547.5716 | www.bodypoint.com

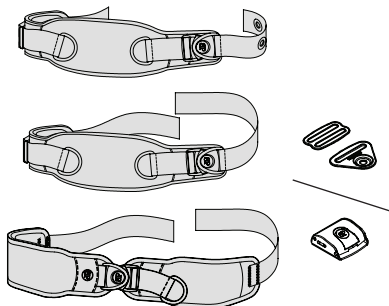

PACKAGE CONTENTS

1 or 2 piece Monoflex™




Mounting straps with Cinch-mount™ or Flat-mount™, or Mounting straps with grommets



POSITIONING




Seat user in wheelchair and establish correct posture with pelvic support belt. Determine desired position for the chest belt.

Position lower over the belly for more freedom of movement – position higher over the chest for more trunk control. When choosing position, consider interference with other devices.

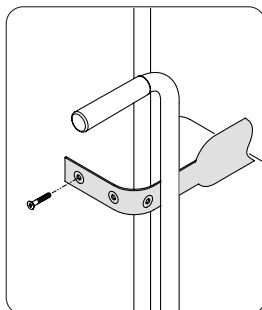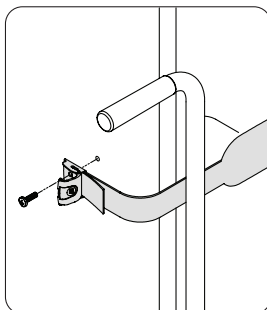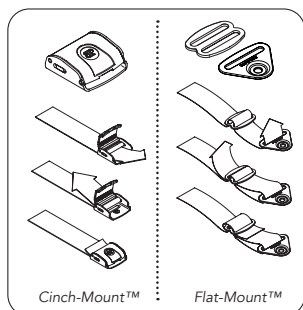

DIRECT SCREW MOUNTING

Mounting straps can be attached directly to solid back surfaces. Use 6mm (1/4") Flat head or Button head screws to mount to chair frame or solid back. Mounting screws must have a minimum pullout strength of 90kg (200lbs). (Not included in package.)



BELT MOUNTING HARDWARE

Mounting straps can be attached using any type of Bodypoint belt mounting hardware with 6mm screws. (HW320 Band Clamps shown, for other types see www.bodypoint.com/hardware.aspx)

ADJUSTMENT

With the user correctly seated, check the fit of the belt – it should be snug so the user is secure. Small adjustments in fit are done using the D-ring tightening straps. Large adjustments in fit are done using the mounting straps.

SAFETY CHECK

When properly positioned in wheelchair, have user lean forward and side to side to check fit. Check for:

1. Normal operation of buckles and adjustment straps.
2. Comfort – If any rubbing occurs relocate straps.
3. Position – If too high or too low, adjust mounting location.
4. Interference with other devices – Relocate straps as necessary to clear armrests, accessory pads, or feeding tubes.